

# PRV

PATENT- OCH REGISTRERINGSVERKET  
Patentavdelningen

PCT/ SE 00/ 0 1 2 8 6

SE00/1286

#2

REC'D 08 SEP 2000

WIPO

PCT

## Intyg Certificate

Härmed intygas att bifogade kopior överensstämmer med de handlingar som ursprungligen ingivits till Patent- och registreringsverket i nedannämnda ansökan.

This is to certify that the annexed is a true copy of the documents as originally filed with the Patent- and Registration Office in connection with the following patent application.

(71) Sökande Olle Inganäs, Linköping SE  
Applicant (s) Edwin Jager, Linköping SE  
Anders Selbing, Linköping SE

(21) Patentansökningsnummer 9902348-3  
Patent application number

(86) Ingivningsdatum 1999-06-21  
Date of filing

Stockholm, 2000-08-16

För Patent- och registreringsverket  
For the Patent- and Registration Office

Åsa Dahlberg  
Åsa Dahlberg

Avgift  
Fee

## PRIORITY DOCUMENT

SUBMITTED OR TRANSMITTED IN  
COMPLIANCE WITH RULE 17.1(a) OR (b)

PATENT- OCH  
REGISTRERINGSVERKET  
SWEDEN

Postadress/Adress  
Box 5055  
S-102 42 STOCKHOLM

Telefon/Phone  
+46 8 782 25 00  
Vx 08-782 25 00

Telex  
17978  
PATOREG S

Telefax  
+46 8 666 02 86  
08-666 02 86

## Kateterburna mikrokirurgiska verktygsset Sammandrag

Användningen av mikrokirurgiska verktygsset, burna på nålar i katetrar, med ett flertal elektriskt drivna mikroverktyg baserade på konjugerade polymerers volymsförändring vid elektrokemisk stimulering. Mikroverktyg kan användas för att hålla strukturer(clips), begränsa flöden genom cylindriska strukturer(clips, pincetter,), förstärka ihåliga cylindrar(stents), expandera strukturer, montera hållare genom membran, hålla cylindriska objekt för elektrisk kontaktering,

The use of microstructures to assemble, separate, fortify, close and hold biological structures inside the body during and after surgery

(stents, valves, clips, nets, knives, scissors, dilators, clamps, tweezers)

### Introduction

The use of microstructures to assemble, fortify or dilate biological structures inside the body during and after surgery can help the surgeon in a number of ways. The operation of electrically actuated tools can relieve the surgeon of the simultaneous tasks of positioning the tool, operating it manually and observing the positioning and operation with some imaging method. By positioning the tool by hand and separately operating it through external control (i.e. footswitch, voice control, other software-control) a much higher degree of precision is expected. In microsurgery, this is an especially desired advantage.

Being able to apply, beforehand or during an invasive procedure, the tool of a required size and geometry - designed for the purpose of cutting, drilling, holding, dilating, suturing, adapting, supporting - from a set of tools that, for example, could be placed in the end of a catheter or needle, is another desired function, requiring development of microactuators.

The application of a tool placed in or introduced through a catheter or needle is of particular interest at the application of structures which are to be left at the site after insertion, and which have to execute their function for some limited time duration. The first example here is that of clips for surgery, sub-millimeter to millimeter structures, which would be used to hold two separated biological structures joined, for example during a healing period (Fig.1).

Another example is that of structures for controlling the flow through blood vessels. The simplest level is that of a clip used to prevent blood flow to a biological structure downstream in the blood flow. Such a clip, or series of clips, would be mounted and left to hold a firm grip on the blood vessel and thus to prevent the flow of blood. In Figure 2 is shown a series of structures suitable for constricting blood vessels.

The third example is at a somewhat more complex level with structures built in a geometry where they could be used inside or outside tube-like structures, as so called stents to dilate a stenotic area or to internally or externally fortify the structure (Figure 1B). Stents are of particular interest since they are to be inserted inside the tube, then to be left there to expand a stenotic or to fortify an area of the tube-like structure.

Arrays of fingers could be used to hold cylindrical objects, such as nerves and nerve fibers, or blood vessels. With the help of microactuators holding the structures (Fig. 3), adjacent microstructures operating as neural sensing or activating electrodes, will enable the reading or stimulation of the nerves. This could be used for a synthetic neural connector, bridging a severed nerve or nerve fiber.

Elements with some temporary mechanical function could be inserted in membranes (Fig.4) Insertion devices of this kind could be used for mounting a hole through a membrane such as commonly used in ear surgery for pressure equilibration. Making these as microdevices will much decrease the effort and nuisance of the inserted devices.

Clips, stents, finger arrays and insertion devices, once applied, could be resorbable or permanent. They could express various degrees of stimulation of cell growth on its surfaces, various degrees of anti-thrombotic activity as well as different anti-biotic activities. They can also be carriers of various biochemical or biological components.

The necessary elements to accomplish these functions are the electrochemically activated micromuscles, built by micromachining thin metal and polymer layers (Elisabeth Smela, Olle Inganäs and Ingemar Lundström: "Controlled Folding of Micron-size Structures", Science 268 (1995) pp.1735-1738). These actuators can be produced in sizes from micrometers to centimeters, and operate well in biological fluids such as blood plasma, blood, buffer and urine. They are therefore suitable tools for micro invasive surgery inside the body. The versatility of construction and the speed of response, as well as the force of these actuators render them as one of the best types of microactuators inside the body. An international patent covers one route of fabrication of such devices (patent A Elisabeth Smela, Olle Inganäs och Ingemar Lundström: "Methods for the fabrication of micromachined structures and micromachined structures manufactured using such methods ", Svensk patentansökan SE 9500849-6,10 mars, 1995 in succession also a PCT and international patent )

#### Prior art

The combination of microactuators and catheters are not well documented in the literature. A patent search reveals a few examples but none that describes the use of microactuators as tools housed inside a catheter; several examples of microactuators use to position a catheter are to be found in the following patents

US5771902: Micromachined actuators/sensors for intratubular positioning/steering

US5819749: Microvalve

WO9837816A1: MICROFABRICATED THERAPEUTIC ACTUATORS

WO9739688A2: METHOD AND APPARATUS FOR DELIVERY OF AN APPLIANCE IN A VESSEL

WO9739674A1: SPRING BASED MULTI-PURPOSE MEDICAL INSTRUMENT

US5855565: Cardiovascular mechanically expanding catheter ).

Several mechanism are suggested for the microactuators in these applications, found among shape memory alloys (also polymeric materials) and piezoelectric materials. The use of conjugated polymers in micromuscles is not documented for catheter tools. Our novelty and innovation therefore resides in the use of microactuators based on conjugated polymers being electrically operated and mounted on a catheter needle, to be positioned with the help of the catheter, and then activating the microactuator structures carried on the needle. The microfabrication of such microactuators renders possible a number of geometries in the range between 10  $\mu\text{m}$  to 1 mm, difficult to produce by mechanical production techniques. They may be produced by patent A above and then mounted on the needle, or they might be produced by novel manufacturing methods. With the help of this invention, completely novel microsurgery tools are available.

The production of individually actuated tool arrays render little difficulty beyond that of producing the individual tool; we have to see that electrical contacts are supplied to actuate each microactuator separately. This can be done by wiring the single microactuator, to be used as the working electrode; the catheter is then used as the counterelectrode, and will be able to supply all the charge we ever need to actuate all those microactuators. As wires may easily be produced in width down to 10  $\mu\text{m}$  with photolithography or with soft lithography, we will be able to put at least 50 microactuators along the tool array located on a needle of 1 mm width, with the simple philosophy of putting down parallel conductor wires. Should we need more, more elaborate addressing schemes might be needed.

Should a necessity for three electrode systems be found in any of the applications, microfabricated reference electrodes or macrosized reference electrodes carried on the catheter housing offers a solution for this problem.

Should the tool arrays be collectively addressed, and the tool array be designed to set free the outermost clip on actuation of all the clips, we will need a mechanism of confining the movements of all but the outermost clip. This is done by assembling the clip array into a cylindrical housing, preferably the catheter, prior to insertion in the body. The cylindrical housing is now confining the motion of microactuators, which search in vain to expand the strong metal casing on operation. When the outermost clip C1 is actuated, the clip is opened; likewise is the next-to-the outermost clip C2 partially free to move as it is protruding outside the cylindrical housing. Therefore the partial opening of C2 sets C1 free, as well as opens it up for subsequent spontaneous closing on the site to be clipped.


#### Figure captions

Figure 1 shows clips and clip arrays, where the clips are mounted in sequence, and area confined by a cylindrical housing, and where the activation of the outer most clip C1 , opening up the clip to join the open structure W1, and then being set free by the simultaneous operation of C2 , so as to be left at the structure W1, holding the structures together.

Figure 2 shows tubular tweezers, tweezers and knives, based on microactuators. The indicated movement is driven by microactuators properly mounted and designed.

Figure 3 shows a neural connector, where a number of small fingers coil around a cylindrical nerve to make a tight hold the the nerve. Two separate nerves are here joined with the help of a common neural connector, which would be desired for accomplishing regrowth of the nerves. In addition, small electrodes can be fashioned along with the microfingers, and be used to sense or excite nerve signals.

Figure 4 An insertion device, for making a (semi)- permanent hole through a membrane. The device is housed in a catheter and is inserted through the membrane so as to make the device form a hole through the membrane.



## CLAIMS

1. Tool arrays for biomedical surgery, characterized in that
  - (i) the tools consist of layered polymer micromuscles arranged to induce geometrical changes and movements via an electrochemically induced change of volume in at least one polymer layer, and
  - (ii) the tool arrays are mounted on a carrier having the form of a needle being inserted into a catheter, which arrays can be electrically actuated via an external means to induce a mechanical movement to act upon biological structures.
2. Tool arrays according to claim 1, characterized in that the layered polymer consists of a single layered polymer.
3. Tool arrays according to claim 1, characterized in that the layered polymer consists of a bi-layered polymer.
4. Tool arrays according to claim 1, characterized in that the layered polymer consists of multilayered polymer and metal layers.
5. Tool arrays according to one or more of claims 1-4, characterized in that the mechanical movement is used to position a biological structure.
6. Tool arrays according to one or more of claims 1-4, characterized in that the mechanical movement is used to hold a biological structure.
7. Tool arrays according to one or more of claims 1-4, characterized in that the mechanical movement is used to cut a biological structure.
8. Tool arrays according to one or more of claims 1-4, characterized in that the mechanical movement is used to dilate a biological structure.
9. Tool arrays according to one or more of claims 1-4, characterized in that the mechanical movement is used to fortify a biological structure.
10. Tool arrays according to one or more of claims 1-4, characterized in that the mechanical movement is used to implant a biological structure.
11. Tool arrays according to one or more of claims 1-10, characterized in that a number of identical tools are located on a tool array extending along the length of the catheter or needle, and wherein the actuation of a tool closest to the exit of the catheter is arranged to release a tool from the tool array and is arranged to leave it at the point of exit of the catheter in order to mount the tool at some biological structure inside a body.
12. Tool arrays according to claim 11, characterized in that a number of identical tools are located on the tool array extending along the catheter or needle and where each tool is arranged to become individually actuated.

13. Tool arrays according to claim 11, characterized in that a number of non-identical tools are located on the tool array extending along the catheter or needle and where each tool is arranged to become individually actuated.

14. Tool arrays according to one or more of claims 1-13, characterized in that the individual tool is a clip arranged to join biological tissues or tissue parts, and arranged to hold the said tissues or tissue parts to allow healing.

15. Tool arrays according to one or more of claims 1-13, characterized in that the individual tool is an expandable cylindrical object designed to be inserted, in a contracted state, into a biological tube, and arranged to become expanded to keep said tube in an expanded state.

16. Tool arrays according to one or more of claims 1-13, characterized in that the individual tool is a scissor.

17. Tool arrays according to one or more of claims 1-13, characterized in that the individual tool is a knife which is arranged on an actuator being arranged for linear and/or angular movement.

18. Tool arrays according to one or more of claims 1-13, characterized in that the individual tool is a sharp needle which is arranged on an actuator being arranged for linear and/or angular movement.

19. Tool arrays according to one or more of claims 1-13, characterized in that the individual tool is a dilator.

20. Tool arrays according to one or more of claims 1-13, characterized in that the individual tool is a clamp.

21. Tool arrays according to one or more of claims 1-13, characterized in that the individual tool is a tweezer.



22. Tool arrays according to one or more of claims 1-21, characterized in that the polymer micromuscles are built of layers, of which at least one is a conjugated polymer.

23. Tool arrays according to claim 22, characterized in that the conjugated polymer is selected from the group consisting of pyrrole, aniline, thiophene, para-phenylene, vinylene, and phenylene polymers and copolymers.



24. Tool arrays according to claim 1, characterized in that the tool is built of bi-layered polymer, where the electrically activated volume change of said at least one conjugated polymer is arranged to cause a bending of said bi-layer.

25. Tool arrays according to claim 1, characterized in that the tool is built of multilayered polymer, where the electrically activated volume change of said at least one conjugated polymer is arranged to cause a bending of said multilayer.

Fig 1B  
Stent

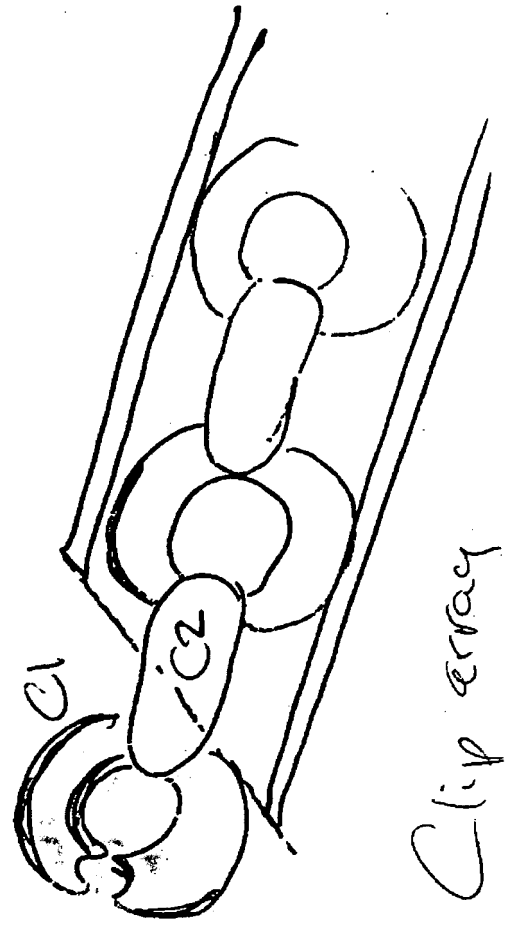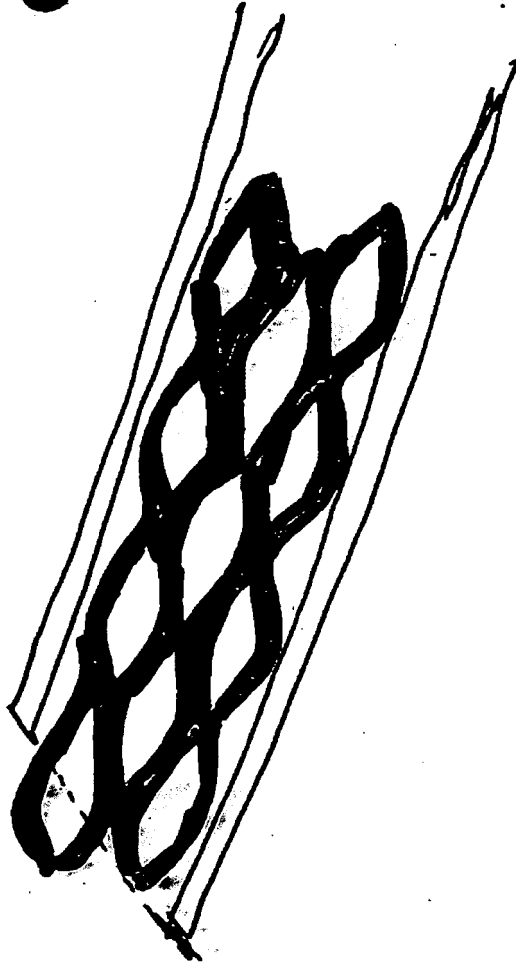

Clip array

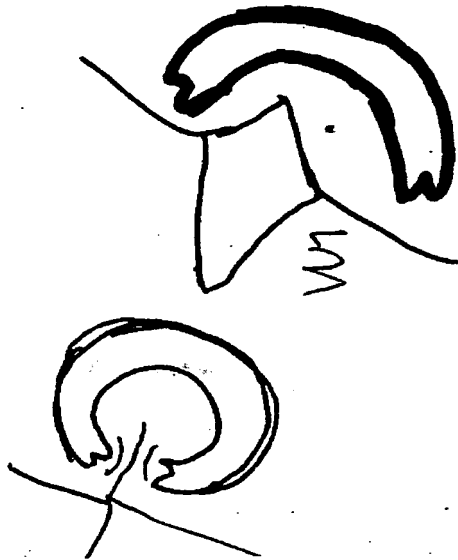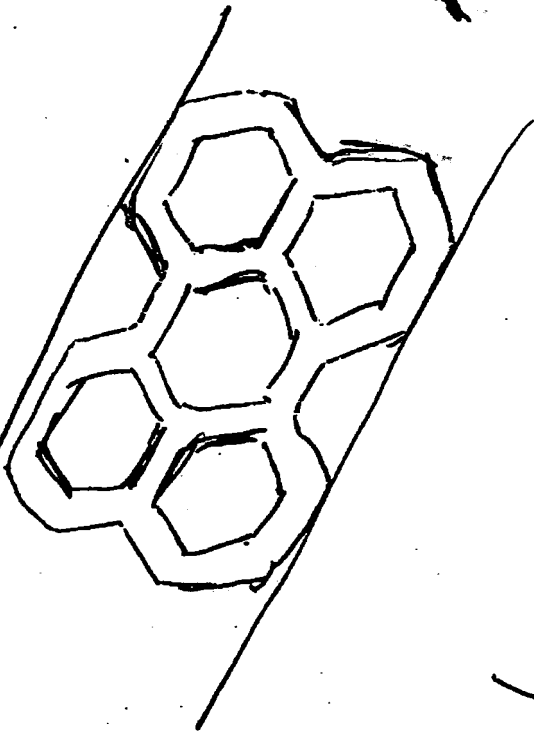

Clip







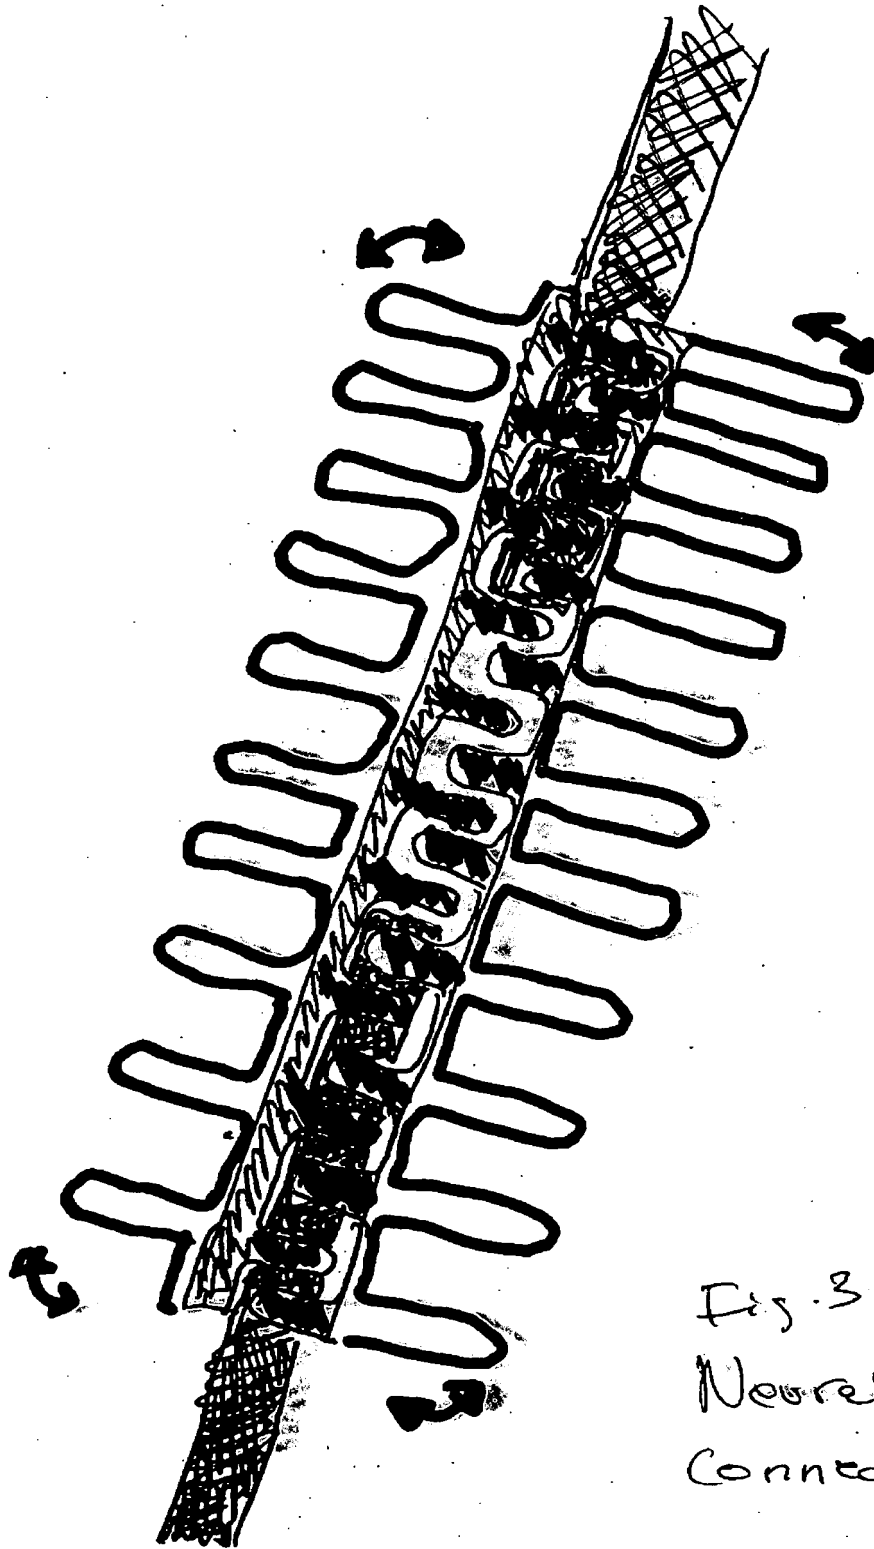


Fig. 3  
Neural  
Connector

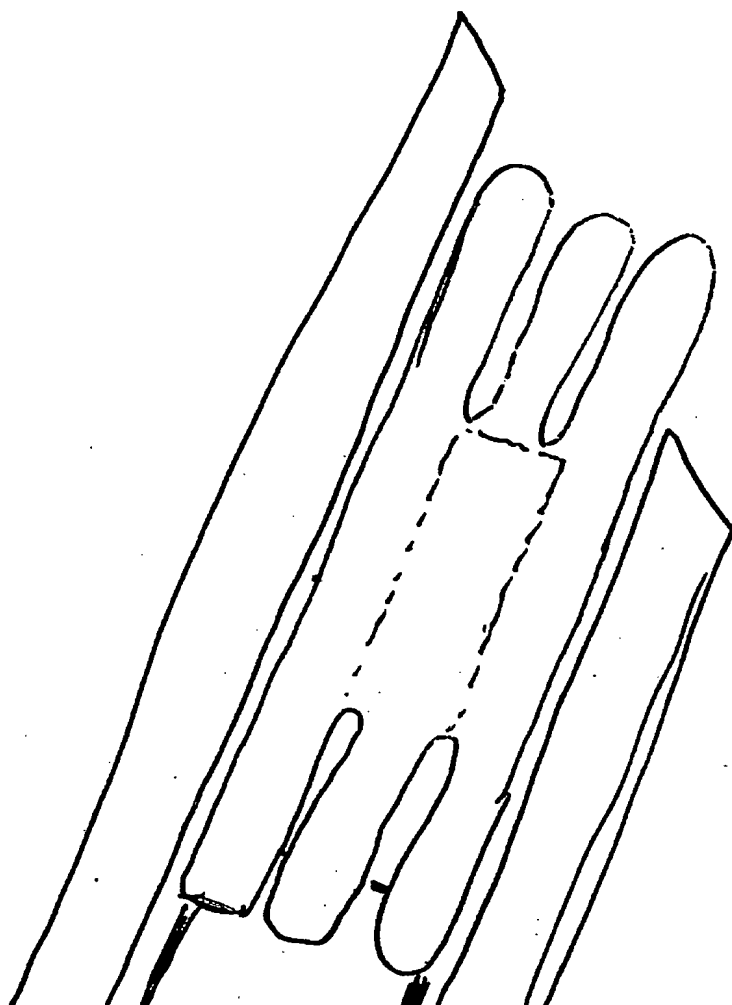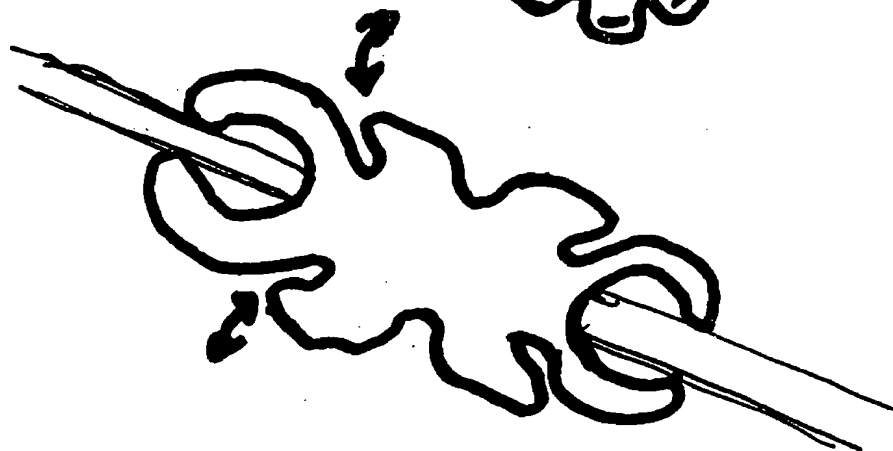

Insertion device

10  
 11  
 12  
 13  
 14  
 15  
 16  
 17  
 18  
 19  
 20  
 21  
 22  
 23  
 24  
 25  
 26  
 27  
 28  
 29  
 30  
 31  
 32  
 33  
 34  
 35  
 36  
 37  
 38  
 39  
 40  
 41  
 42  
 43  
 44  
 45  
 46  
 47  
 48  
 49  
 50  
 51  
 52  
 53  
 54  
 55  
 56  
 57  
 58  
 59  
 60  
 61  
 62  
 63  
 64  
 65  
 66  
 67  
 68  
 69  
 70  
 71  
 72  
 73  
 74  
 75  
 76  
 77  
 78  
 79  
 80  
 81  
 82  
 83  
 84  
 85  
 86  
 87  
 88  
 89  
 90  
 91  
 92  
 93  
 94  
 95  
 96  
 97  
 98  
 99  
 100  
 101  
 102  
 103  
 104  
 105  
 106  
 107  
 108  
 109  
 110  
 111  
 112  
 113  
 114  
 115  
 116  
 117  
 118  
 119  
 120  
 121  
 122  
 123  
 124  
 125  
 126  
 127  
 128  
 129  
 130  
 131  
 132  
 133  
 134  
 135  
 136  
 137  
 138  
 139  
 140  
 141  
 142  
 143  
 144  
 145  
 146  
 147  
 148  
 149  
 150  
 151  
 152  
 153  
 154  
 155  
 156  
 157  
 158  
 159  
 160  
 161  
 162  
 163  
 164  
 165  
 166  
 167  
 168  
 169  
 170  
 171  
 172  
 173  
 174  
 175  
 176  
 177  
 178  
 179  
 180  
 181  
 182  
 183  
 184  
 185  
 186  
 187  
 188  
 189  
 190  
 191  
 192  
 193  
 194  
 195  
 196  
 197  
 198  
 199  
 200  
 201  
 202  
 203  
 204  
 205  
 206  
 207  
 208  
 209  
 210  
 211  
 212  
 213  
 214  
 215  
 216  
 217  
 218  
 219  
 220  
 221  
 222  
 223  
 224  
 225  
 226  
 227  
 228  
 229  
 230  
 231  
 232  
 233  
 234  
 235  
 236  
 237  
 238  
 239  
 240  
 241  
 242  
 243  
 244  
 245  
 246  
 247  
 248  
 249  
 250  
 251  
 252  
 253  
 254  
 255  
 256  
 257  
 258  
 259  
 260  
 261  
 262  
 263  
 264  
 265  
 266  
 267  
 268  
 269  
 270  
 271  
 272  
 273  
 274  
 275  
 276  
 277  
 278  
 279  
 280  
 281  
 282  
 283  
 284  
 285  
 286  
 287  
 288  
 289  
 290  
 291  
 292  
 293  
 294  
 295  
 296  
 297  
 298  
 299  
 300  
 301  
 302  
 303  
 304  
 305  
 306  
 307  
 308  
 309  
 310  
 311  
 312  
 313  
 314  
 315  
 316  
 317  
 318  
 319  
 320  
 321  
 322  
 323  
 324  
 325  
 326  
 327  
 328  
 329  
 330  
 331  
 332  
 333  
 334  
 335  
 336  
 337  
 338  
 339  
 340  
 341  
 342  
 343  
 344  
 345  
 346  
 347  
 348  
 349  
 350  
 351  
 352  
 353  
 354  
 355  
 356  
 357  
 358  
 359  
 360  
 361  
 362  
 363  
 364  
 365  
 366  
 367  
 368  
 369  
 370  
 371  
 372  
 373  
 374  
 375  
 376  
 377  
 378  
 379  
 380  
 381  
 382  
 383  
 384  
 385  
 386  
 387  
 388  
 389  
 390  
 391  
 392  
 393  
 394  
 395  
 396  
 397  
 398  
 399  
 400  
 401  
 402  
 403  
 404  
 405  
 406  
 407  
 408  
 409  
 410  
 411  
 412  
 413  
 414  
 415  
 416  
 417  
 418  
 419  
 420  
 421  
 422  
 423  
 424  
 425  
 426  
 427  
 428  
 429  
 430  
 431  
 432  
 433  
 434  
 435  
 436  
 437  
 438  
 439  
 440  
 441  
 442  
 443  
 444  
 445  
 446  
 447  
 448  
 449  
 450  
 451  
 452  
 453  
 454  
 455  
 456  
 457  
 458  
 459  
 460  
 461  
 462  
 463  
 464  
 465  
 466  
 467  
 468  
 469  
 470  
 471  
 472  
 473  
 474  
 475  
 476  
 477  
 478  
 479  
 480  
 481  
 482  
 483  
 484  
 485  
 486  
 487  
 488  
 489  
 490  
 491  
 492  
 493  
 494  
 495  
 496  
 497  
 498  
 499  
 500  
 501  
 502  
 503  
 504  
 505  
 506  
 507  
 508  
 509  
 510  
 511  
 512  
 513  
 514  
 515  
 516  
 517  
 518  
 519  
 520  
 521  
 522  
 523  
 524  
 525  
 526  
 527  
 528  
 529  
 530  
 531  
 532

**This Page Blank (uspto)**